


KONA | XM

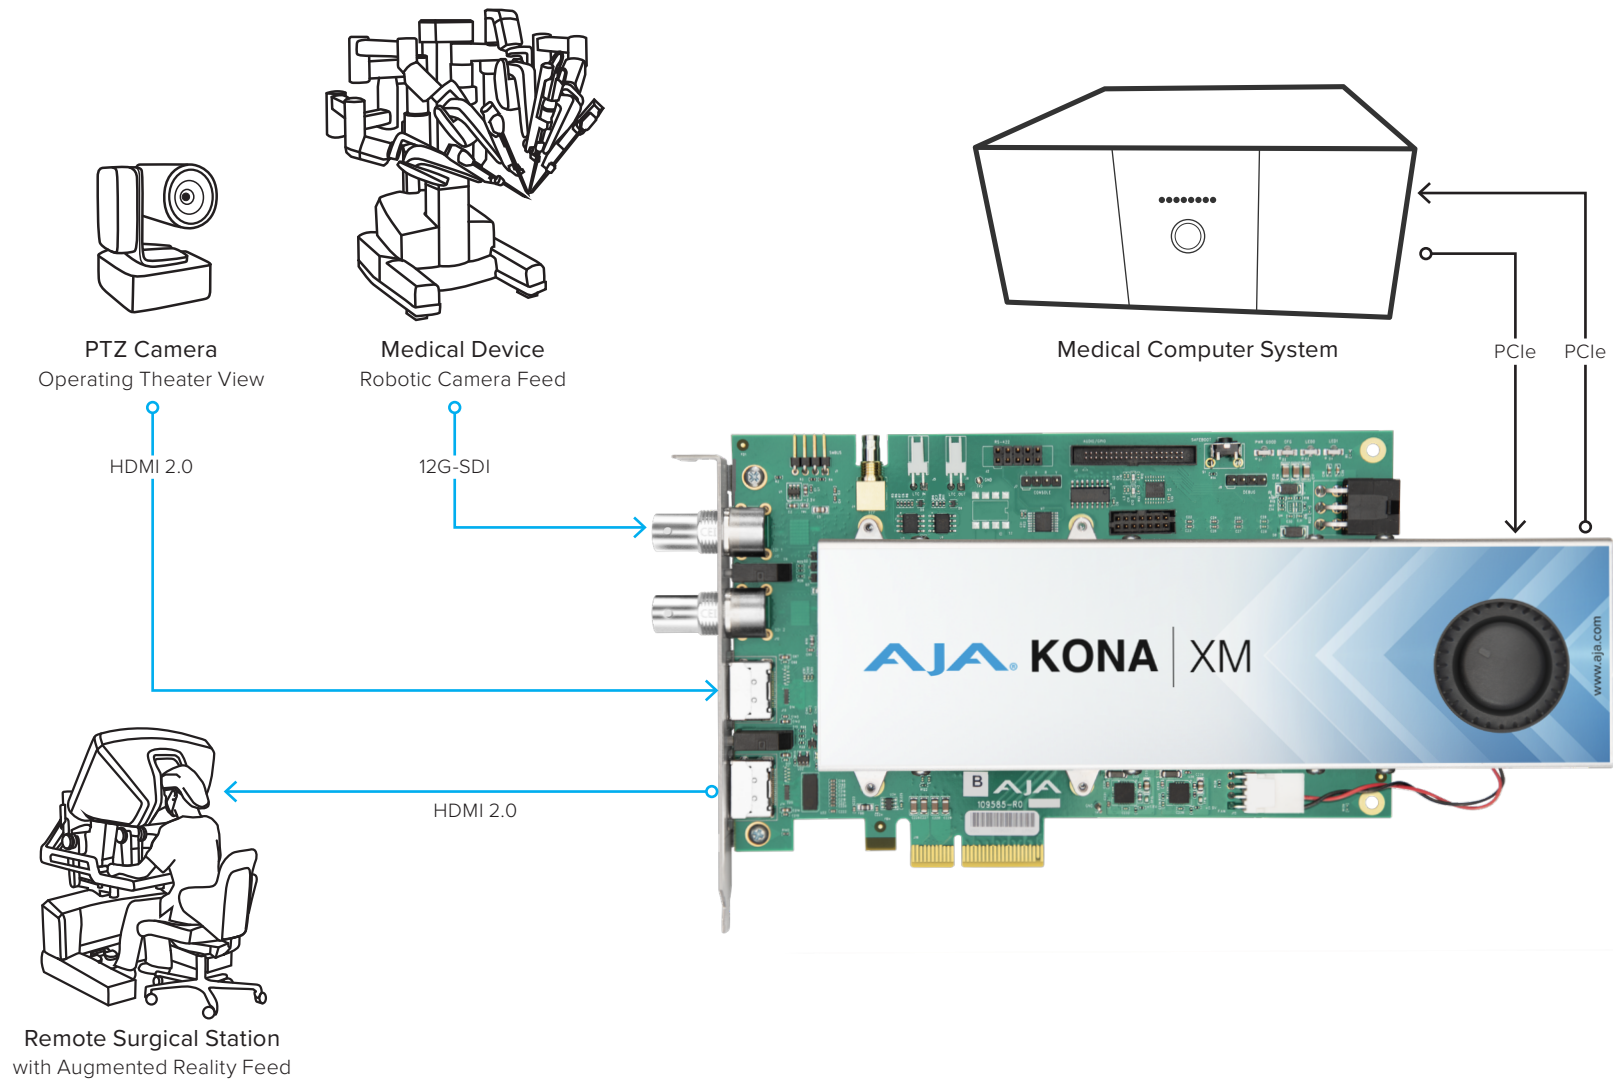

AI/AR Assisted Surgery Workflow with KONA XM

NOTE: When using HDMI input, SDI output will only be possible if HDMI input video is a supported SDI mode, and HDMI signals meet SDI timing constraints.